PetNAD

Leptospirosis (lipL32) Detection Kit

For leptospirosis

User Manual

For Research Use Only

Manufacturer:

GeneReach Biotechnology Corporation

TEL: 886-4-24639869 FAX: 886-4-24638255

No. 19, Keyuan 2nd Road, Central Taiwan Science Park, Taichung City, Taiwan 407

Web Site: www.petnad.com

2014/09

Content

INTENDED USE1				
SCI	ENTIFIC MEANINGS	1		
SUI	MMARY AND EXPLANATION	2		
PRI	INCIPLES OF THE PROCEDURE	3		
PRO	ODUCT DESCRIPTION	3		
A.	Materials Provided	.3		
B.	Materials and Equipments Required, but Not Provided	.4		
C.	Storage and Stability	.4		
D.	Sample Type	.4		
RE	COMMENDED NUCLEIC ACID EXTRACTION METHOD	S		
•••••		5		
PRI	ECAUTIONS	5		
LIN	/ITATIONS	6		
PRO	OCEDURE	8		
A.	PetNAD [™] Leptospirosis <i>lipL32</i> Detection Kit Quick Guide	.8		
B.	Procedure	.9		
DA'	TA INTERPRETATION1	1		

PetNADTM Leptospirosis (lipL32) Detection Kit

ANALYTICAL SENSITIVITY	11
TROUBLESHOOTING	
REFERENCE	14

INTENDED USE

PetNADTM Leptospirosis (*lipL32*) Detection Kit is intended for *in vitro* detection of Leptospirosis DNA based on insulated isothermal polymerase chain reaction (iiPCR) technology. This kit is designed specially to be used with an insulated isothermal (iiPCR)-compatible instrument, **POCKITTM** Nucleic Acid Analyzer. The assay is intended for use by veterinarians or technicians with basic laboratory skills.

This kit is intended for research use only.

SCIENTIFIC MEANINGS

Antibody induced by vaccine or obtained from maternal immunity could lead to false positive interpretation in antibody-based diagnostic procedures. Detecting pathogen's nucleic acids, not antibody, PCRbased methods can avoid the false positive results described above.

Furthermore, with higher analytical sensitivity, PCR can detect lower levels of viral signals than most if not all diagnostic methods. It can reduce the chance of false negative results at early infection stage and shorten the window period between time of infection and detection.

SUMMARY AND EXPLANATION

Leptospirosis, an emerging infectious disease in humans and dogs, is a worldwide zoonotic disease caused by infection with the motier spirochetal bacterium of the genus, *Leptospira* (Bharit et al., 2003). There are over 250 pathogenic serovars based on difference in the carbohydrate component of the bacterial lipopolysaccharide (Levett, 2001; Ko, Goarant, Picardeau, 2009). Different serovars are adapted to different wild or domestic animal reservoir hosts.

Leptospirosis in dogs often occur with signs of renal or hepatic failure, uveitis, pulmonary hemorrhage, acute febrile illness, or abortion (Sykes et al., 2011). Leptospirosis is transmitted by urine of an infected animal, outbreaks of disease in dogs often follow periods of high rainfalls.

PCR is one of the most commonly accepted methods that provide high sensitivity and specificity for leptospirosis detection. However, conventional PCR assays could take three to four hours and require sophisticated thermocyclers and well-trained technicians to perform. GeneReach has developed **PetNADTM** Leptospirosis (*lipL32*) Detection Kit based on iiPCR technology, which significantly reduces reaction time and offers sensitivity and specificity comparable to those of conventional nested PCR (Tsai, 2012; Chang, 2012). Furthermore, this simple and easy assay is completed rapidly in a portable **POCKITTM**

Nucleic Acid Analyzer.

PRINCIPLES OF THE PROCEDURE

In iiPCR, hydrolysis probe-based chemistry is used to generate fluorescent signal during amplification of target DNA. The primers and probe target the *lipL32* gene and do not cross-react with nucleic acid from host and non-pathogenic *Leptospira* spp.

PRODUCT DESCRIPTION

Component Conten		Contents or Purpose	Amount
Premix Pack		Leptospirosis Premix	24 bags (1 leptospirosis
		(lyophilized pellet) containing	Premix vial and 1
		dNTPs, primers, probe, and	desiccating agent/bag)
		enzyme for amplification.	
		Desiccating agent pack.	
Premix Buffer		Reaction buffer to re-dissolve	2 vials (1.3 ml/vial)
В		the lyophilized pellet.	
P(+) Control	P(+) Control Dried plasmid containing		1 vial
		leptospirosis partial sequence	
		as positive control.	

A. Materials Provided (24 tests/kit)

P(+) Control	Reaction buffer to re-dissolve	1 vial (110 µl/vial)
Buffer	P(+) Control.	
R-tube		1 bag (24 pieces/bag)
Сар		1 bag (24 pieces/bag)
User Manual		1 сору

PetNAD[™] Leptospirosis (*lipL32*) Detection Kit

B. Materials and Equipment Required, but Not Provided

- PetNADTM Nucleic Acid Co-prep Kit or tacoTM Automatic Nucleic Acid Extraction System.
- POCKITTM Nucleic Acid Analyzer (POCKITTM): PetNADTMcompatible instrument.
- 3) **cubeeTM** Mini-Centrifuge (**cubeeTM**).
- 4) Micropipette and filter tips.

C. Storage and Stability

- 1) The kit should be stored at 4°C and is stable until the expiration date stated on the label.
- 2) Store Premix vials in sealed Premix Pack to avoid hydration of lyophilized components.
- Reconstituted P(+) Control is stable for 6 months at 4°C. Aliquot reconstituted P(+) Control to avoid degradation of nucleic acid.

D. Sample Type

Nucleic acid extracted from whole blood or urine.

RECOMMENDED NUCLEIC ACID EXTRACTION METHODS


- A. PetNADTM Nucleic Acid Co-prep Kit.
- **B.** taco[™] DNA/RNA Extraction Kit, compatible instrument taco[™] Automatic Nucleic Acid Extraction System.

Note: Please follow the instruction manual of above extraction methods to obtain optimal results. It is the user's responsibility to validate the combination of this reagent set with nucleic acids extracted by other methods for any particular application.

PRECAUTIONS

- A. Do not open R-tube(s) after reaction to prevent any carryover contamination.
- B. Perform extraction and amplification in two independent spaces to minimize contamination.
- C. Do not reuse R-tube and Premix.
- D. Include the P(+) Control to:
 - 1) Ensure **POCKITTM** is working normally.
 - 2) Ensure detection kit performance after storage.

- E. To get optimal fluorescence detection.
 - Wear powder-free gloves to handle R-tubes.
 - Do not label in the detection area of R-tube.




LIMITATIONS

- A. The test should be used only for testing nucleic acid extracted from animal specimens. Do not add specimens (*e.g.* whole blood) directly into Premix.
- B. PetNAD[™] Nucleic Acid Co-prep Kit and taco[™] mini Automatic Nucleic Acid Extraction System are recommended for nucleic acid extraction.
- C. Any deviations from the recommended procedure may lead to suboptimal results. Quality of the extracts should be validated by the users.
- D. For **PetNADTM** Leptospirosis (*lipL32*) Detection Kit, it is strongly recommended to use freshly prepared nucleic acid (within 1 hour after extraction) to achieve optimal results.
- E. Vaccination with a modified-live leptospirosis vaccine may result in positive PCR results for a few weeks after vaccination. Killed or vectored-recombinant vaccines will not interfere with PCR testing.
 PetNADTM is recommended in sick animals with clinical signs

and/or laboratory abnormalities consistent with infection or in an animal with a suspected subclinical infection as based upon history, physical examination and clinical laboratory findings.

PROCEDURE

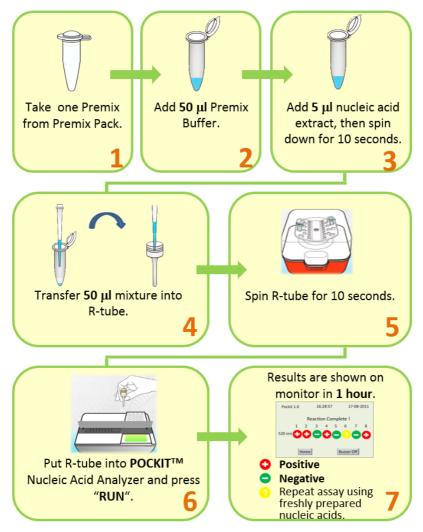

A. PetNADTM Leptospirosis (*lipL32*) Detection Kit Quick Guide

B. Procedure

Note: Before preparing the reactions for iiPCR testing, turn on POCKITTM to initiate the calibration for the instrument. The device will complete self-test within 5 minutes. Please refer to the user manual of POCKITTM for further details.

Note: Before using for the first time, add 100 μ l P(+) Control Buffer to P(+) Control. Store reconstituted P(+) Control at 4°C.

- 1) Label R-tube(s) in the label area.
- Prepare one Premix for each sample. (Premix tube is in Premix Pack. Each Premix Pack contains one Premix tube.)

Note: When the pellet is not found at the bottom of the tube, spin tube briefly to bring it down.

- 3) Add 50 µl Premix Buffer B to each Premix tube.
- Add 5 μl nucleic acid extract or P(+) Control to each Premix tube. Spin Premix tube for 10 seconds in a mini centrifuge (such as cubeeTM).
- 5) Transfer 50 µl Premix/sample mixture into R-tube.
- 6) Seal top of each R-tube with a cap. Make sure R-tube is capped tightly.
- 7) Place R-tube into the holder of **POCKITTM**.
- 8) Spin tube briefly in **cubeeTM** to make sure all solution is

collected at the bottom of R-tube.


Note: Make sure there are no bubbles in the solution.

Note: Start reaction within 1 hour (to prevent nucleic acid degradation and non-specific reaction).

- 9) **POCKITTM** reaction:
 - a) Select "520 nm".
 - When "System READY" is displayed, place the holder with R-tube(s) into the reaction chamber.
 - c) Tap cap of each R-tube to make sure the tube is positioned properly.
- 10) Close lid and press "Run" to start reaction program.
- 11) Test results are shown on the monitor after reaction is completed.

DATA INTERPRETATION

* One example of results shown on the monitor.

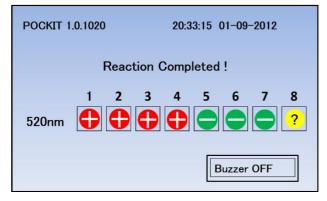

520 nm	Interpretation		
Leptospirosis Positive.			
	Leptospirosis Negative.		
?	Repeat reaction with freshly prepared nucleic		
	acid.		

ANYLYTICAL SENSITIVITY

The detection limit of **PetNADTM** Leptospirosis (*lipL32*) Detection

Kit is about 10 copies/reaction.

TROUBLESHOOTING

Problems	Possible causes	Solutions
False Positive	1) Reuse of micro- centrifuge tubes, tips, R-tubes and Premix.	 Micro-centrifuge tubes, tips, R-tubes and Premix are for single-use only. Reusing these accessories would cause cross-contamination, and therefore false positive results. Used micro-centrifuge tubes, tips, R-tubes and Premix should be collected and discarded according to local regulation. Do not place the waste close to the working area to prevent cross-contamination.
	2) Contaminated micropipette	■ Use aerosol-free tips.
	3) Contaminated reagent	 Consult with a GeneReach technical support representative or local distributor.
	 Contaminated working area 	Consult with a GeneReach technical support representative on how to clean up working area.

Problems	Possible causes	Solutions
False	1) Nucleic acid	Consult manual of nucleic acid
Negative	extraction failed.	extraction kit.
	2) PCR inhibition	Do not overload PCR with too
		much nucleic acid.
		 Spike nucleic acid sample (5 μl)
		into a P(+) Control reaction for a
		parallel PCR reaction. Negative
		results indicate the presence of
		inhibitors in the nucleic acid. In
		that case, prepare another nucleic
		acid extract.
Heavy	1) Leakage or spill of	Consult with a GeneReach
contamination	reaction from R-	technical support representative or
of amplicons	tube into reaction	local distributor.
in reaction	chamber of	
chamber of	РОСКІТтм.	
РОСКІТтм.		

REFERENCE

- 1. Bharti, A.R., Nally, J.E., Ricaldi, J.N., et al., (2003). Leptospirosis: a zoonotic disease of global importance. Lancet Infect Dis;3(12):757–71.
- Chang, H.F. G., Tsai, Y.L., Tsai, C.F., Lin, C.K., Lee, P.Y., Teng, P.H., Su, C. and Jeng, C.C., (2012). A thermally baffled device for highly stabilized convective PCR. *Biotechnology Journal* 7(5): 662-666, doi: 10.1002/biot.201100453
- 3. Levett, P.N., (2001). Leptospirosis. Clin Microbiol Rev 14:296–326.
- 4. Ko, A.I., Goarant, C., Picardeau, M., (2009). Leptospira: The dawn of the molecular genetics era for an emerging zoonotic pathogen. Nat Rev Microbiol 7:736–747.
- Sykes J.E., Bryan J., Amstrong P.J., (2011). 2010 ACVIM Small Animal Consensus Statement on Leptospirosis:Diagnosis, Epidemiology, Treatment, and Prevention. J Vet Intern Med 2011;25:1–13.
- Tsai Y.L., Wang H.T.T., Chang H.F.G., Tsai C.F., Lin C.K., Teng P.H., Su C. and Jeng C.C., (2012) Development of TaqMan probe-based insulated isothermal PCR (iiPCR) for sensitive and specific on-site pathogen detection. *PLoS ONE* 7(9): e45278. doi: 10.1371/journal.pone. 0045278